

MODEL BASED CONTROL FOR INSULIN INFUSION SYSTEM IN POSTOPERATIVE DIABETIC PATIENTS – A NOVEL APPROACH

A.Alavudeen Basha, Dr. S. Vivekanandan,

Research Scholar, Associate Professor, IEEE, VIT University, Vellore

ABSTRACT:

In post-operative period, the variation of the blood glucose level is one of the important complications to be controlled which avoid abnormal conditions like hypo/hyper glycaemia that leads to emergency situation [1]. To overcome this condition the closed loop control strategy is used to infuse the insulin to the human body as a continuous infusion system that stabilizes its level. In this paper two different model based controllers (Model Predictive control and Internal Model Control) were designed and their performances were observed. The output of the controller were compared and tested with Bergman minimal model in normal condition and even with series disturbance like meal and exercise. [6] The results clearly predict that model predictive controller performance is better and meets the target.

Key Words: Diabetic infusion system, Minimal model, Model predictive control, internal model control.

INTRODUCTION:

The increment or decrement to the basal value is called hypo/hyperglycemia state which is dangerous, of that hypoglycemia is a more serious and it can cause coma or may be even fatal. Hypoglycemia is a well-known complication for cardiac surgery patients and a study clearly depicts that the glucose levels were high which was reviewed from 1,586 patients of vascular surgery 560 (36%) persons, 227 (14%) had colon related surgery and 779 (50%) were part of surgical procedure [1]. The literature survey portrays that researches have made an attempt to find various methods to treat the post-operative patients and one of the common traditional method is closed loop insulin delivery system (Artificial Pancreas) that is capable of maintaining glucose level for diabetic patient with the desired level of insulin delivery [6].

The insulin infusion system is an integrated system contains synthetic materials as per the medical standards, which will substitute the pancreas with sensing the blood glucose and calculate the desired amount of insulin required and deliver the desired amount to the human body with the help of insulin pump. Fig.1 shows the basic architecture of the closed loop insulin control system, in which the controller regulates the details between the sensor input and desired insulin range [10].

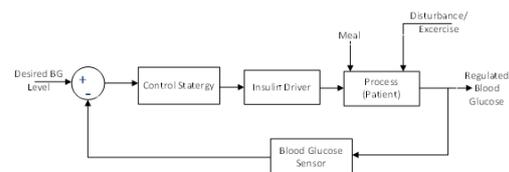


Fig.1: Closed loop drug delivery control structure

The control algorithm is used based on the optimal requirement and the controller input given to insulin pump with the help of syntactic micro needle. In this paper the proposed closed loop control strategy will produce the output equal to the pancreas and this research is keen to develop the system which will produce the optimal insulin infusion.

1. MATERIALS AND METHODS:

The mathematical model describes the dynamics of the human diabetic system that helps to find the correlation between the insulin and its resistance also helps to design the control system based on standard rules and measures [5]. Basically the human body is a nonlinear stochastic and intrinsic system of that pancreas is an independent system that controls the blood glucose level. When pancreas does not work properly, insulin has to be pumped artificially to the patient which plays an important role called artificial pancreas [7].

During the last decades, an interesting number of mathematical models has been developed based on the non-exhaustive criteria [9], the different aspects of diabetes [11], including glucose-insulin dynamics, beta-cell function [12], epidemiology of diabetes [16], management and the burden of diabetes and its complications [10]. Prof. Bergman an awardee of the American Diabetes Association (2006) for his achievements in the development of the famous minimal model (Fig.2) for diabetes that indicates the importance of mathematical model in the basis of diabetes and its management.

Based on the observation the parameters has taken for an steady state process with approximate parameters and the model designed based on the selected approximate values, also these models limited with real time prediction of the glucose measurement . The observation of frequently measured data with insulin availability, glucose compactness along with sensor system errors [9].

$$\frac{dG_m(t)}{dt} = -p_1 [G_m(t) - G_b] - x(t)G_m(t) + [d(t) + C(t)] \quad (1)$$

$$\frac{dX}{dt} = -p_2X(t) + p_3 I \quad (2)$$

$$\frac{dI_d(t)}{dt} = -n[I(t) - I_b] + \gamma[G_m(t) - h] + r(t) \quad (3)$$

In the model $G_m(t)$ is noted as plasma glucose concentration (mg/dl) and $I(t)$ denotes insulin concentration (μ U/ml), The I_b is considered as basal value of insulin level (mU/L) and $X_i(t)$ is observed as insulin in plasma glucose, $U(t)$ is called as external input insulin (mU/min) and $D_i(t)$ is external input glucose of the human body (mm/min). I_b and G_b are glucose and insulin concentration before infusion of the insulin. The P_1, P_2, P_3 , are patient parameters taking as random and 'n' is change in rate of insulin, which is used in plasma layer (Min^{-1}). Bergman theory denotes the values of the parameters [11], P_1, P_2 and P_3 , may be regulates based on the different conditions the values are $P_1=0, P_2=0.025, P_3=0.000013$ and for Type 1 diabetic patient and the values can be identified as follows P. For normal person, the values are $P_1=28/1000, P_2=25/1000, P_3=0.000013$ [9, 12].

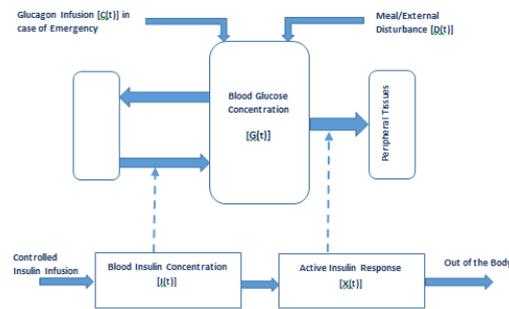


Fig.2: Bergman Minimal Model System Architecture

Based on the values and equations, Lynen and Bequette developed a diabetic model process transfer function (6) along with the process parameters [23].

$$Gp_g(s) = \frac{-3.79}{(40s+1)(10.8s+1)} \quad (4)$$

Also the transfer function with meal to be consider as follows

$$Gd_m(s) = \frac{8.44}{s(20s+1)} \quad (5)$$

The meal difference is consider as pulse value, the 5- Gm glucose meal consumed in 15 min tile lag, the pulse is developed with the scale of 3.33g/min with the same duration.

2. CONTROLLER SCHEME:

2.1 Model Predictive controller

Model Predictive controller (MPC) is an advanced control technique used in process industries since 1980. As MPC offers several important advantages such as fast response, accurate model prediction, multiple input/output processes in a systematic manner, controlled optimal set point, dynamic model relay and dynamic principles these controllers are used in bio control field [16].

MPC can handle the constraints of the process variables and it can be manipulated and controlled by the variables in a systematic manner for an multivariable control problems naturally, Also it is an easy to tune method

[22], it is a totally open methodology based on certain basic principles which allow for future extensions [15]. The controller schemes are based on the running process of the measurement and the process output is to be responsible on the predictions of the values in future condition. The MPC controller calculations are based on predicted system variables at present condition with the sequence of regulated changes and the controlled changes has been manipulated in the prediction and it will move the set point in an optimal manner and the control technique is shown in Fig.3.

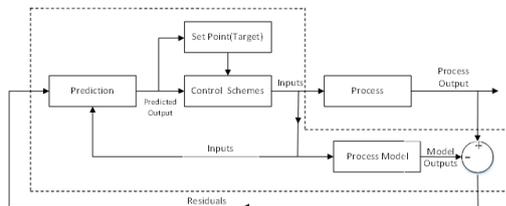


Fig.3: Architecture of Model predictive control System

If the process is probably accurate with the dynamic model of the system and the model, current measurements can be used to predict the values of the process output. The attained changes may be an individual input variables of process model [19]. MPC is implemented based on discrete time nonlinear process models, so the mathematical description can be represented as

$$x_{k+1} = f(x_k, u_k) \quad (6)$$

The MPC control problem is as follows with the knowledge of current output y_k

$$J = \phi(y_k + N_k) + \sum_{j=0}^{N-1} L(y_k + j|k, u_k + j|k, \Delta u_k + j|k) \quad (7)$$

The variable N-move is the control sequence that minimizes the objectives and the measurement is available the parameters of the problem are updated and a new optimization problem is formulated whose solution provides the next control. This recurrent optimization is using to obtain the function and modified through the entire process feedback of MPC to control the variables.

2.2 Internal Model Control

The Internal Model Control (IMC) is an advanced control strategy commonly used in industrial application and controller algorithm is simple and robust to handle the nonlinear and inaccuracies in the process. The IMC controller is contain the specific locating process of the controller performance also the controller is taking the specific control track of the process for an set point of the process, also the IMC controller is contain the explicit filter technique to reject the disturbance for the steady state processes [21]. The Internal Model Control system structure shown in Fig.4 with three different positions. The main part of the controller is used to forecast the process output [24] of the system. The following is the internal loop which is used to differentiate the process output and the internal model output. To end, the third position of the controller can be used to control the error to compute the upcoming values of the process outputs [25].

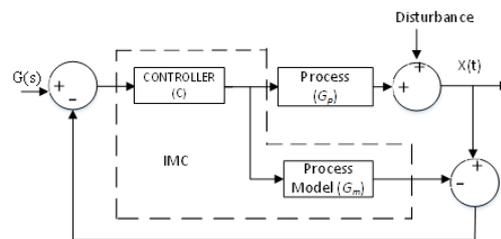


Fig.4 Diagram of IMC structure

The difference between the output of the internal model and the process output is fed back to produce the error, used by the controller. This helps to reduce the effect of disturbances on the system [22]. In this model we have implemented the IMC developed by Garcia and his co-authors [25] on the patient model proposed by Slate and his co-authors [26]. The IMC has been applied to control of blood Glucose in [28]. The conventional IMC structure is shown in Fig.4, in that the parameter G_p is the plant to be controlled and G_m is a plant model of the process, C is the controller based on model control and $x(t)$ is the system output and D is the external disturbance of the system.

Based on the parameters the formulae evaluated as follows,

$$K_{cp} = \frac{2\tau + \tau_d}{2(\lambda + \tau_d)} \quad (8)$$

Where $\tau_d = \frac{\tau \tau_d}{2\tau + \tau_d}$

3. EXPERIMENTAL RESULTS AND DISCUSSION:

The results obtained from MPC and IMC controllers were simulated; tested and compared that predicts and evaluates the optimal infusion of insulin to the human body

The simulation has been carried out with the help of MATLAB with virtual patient model to regulate the desired optimal level of infusion along with the meal disturbance. The IMC and MPC controllers were verified based on the designed parameters and the response of each model was obtained in the presence of disturbances along with meal input. These results are shown (Table 1 and 2), the performance of the controllers are satisfied with both the MPC and IMC controller with the desired level of infusion control. However, the settling time for the IMC control of the patient's responses are shorter than with MPC, especially the multiple disturbance response which has a minimum settling time hat offered by the IMC controller.

Meal Duration	IMC Controller mg/dl	MPC Controller mg/dl
Break Fast	93-138	85-132
Lunch	80-139	82-128
Dinner	85-148	85-135

Table 1: Glucose Prediction level for IMC and MPC Controller

Meal Duration	IMC Controller mU/min	MPC controller mU/min
Break Fast	1.2-5	1.3-5
Lunch	0.6-5	0.8-5
Dinner	1.2-5	0.8-5

Table 2: Insulin Infusion level for IMC and MPC Controller

The tuning parameters are injected in IMC and MPC controllers which is used to control the blood glucose system. The Fig.5 shows the glucose and insulin outputs of IMC controller, based on the output response, the blood glucose increases depends on the meal inputs, similarly the insulin also increases to bring back the blood glucose level to normal condition, in that scenario the response time is lagging due to controller action with the disturbed output, similarly this trend continues for multiple meals and the insulin level also changes and reaches the maximum level. To overcome the disturbance Model Predictive Controller is used, the glucose and insulin response are shown in Fig.6. The MPC allows the disturbance and minimize the sudden change and it bring

backs the blood glucose concentration in minimum level with optimal glucose infusion at the desired level.

As per the design the MPC controller maintain the glucose in the desired level while it increases after the surgical procedures and it will control naturally with pancreas to inject the insulin to our body to maintain the glucose level with the proper controlled delivery, whereas his trend continues for multiple meals and the insulin level also changes and reaches the desired level .The Fig.7 and Fig.8 shows the comparison of IMC and MPC controller glucose level and insulin responses in this the MPC controller gives minimum time to reach the measurement and the controller taken the lesser time to regulate the blood glucose based on the optimal insulin infusion rate.




Fig 5: Response of Glucose vs Insulin Evaluation for IMC controller






Fig 6: Response of Glucose vs Insulin Evaluation for MPC controller



4. CONCLUSION:

In this paper the IMC and MPC controllers were proposed for control the blood glucose system for post-operative patients .The simulation was carried out with reference to diabetic model from which glucose and insulin kinetics were referred with the help of new control strategy carried out and developed, the meal (glucose) is taken as a disturbance and based on the feedback the controlled insulin is infusing to the patient which maintains the glucose level in the body. The simulation of the physiological results of the IMC and MPC controllers are compared and identified the superiority of characteristics are shown and discussed. The optimal selection of parameters in MPC regulates the blood glucose level effectively compared with IMC controller. The controller settings are adopted using a

self-tuning strategy and the settings has been simulated with the minimal model.

This output is a major exertion to develop the model based strategy of continuous glucose control for insulin pumps. The MPC is an effective model based control which requires exact model of blood glucose system, and it will vary patient to patient based on the modelling.

REFERENCE:

- [1] American Diabetes Association (2011) Diagnosis and classification of diabetes mellitus, *Diabetes Care*. 34: S5-S10.
- [2] Theresa Breithaupt., "Postoperative glycemic control in cardiac surgery patients", *harmacology Notes*, pp. 79-82, 2010.
- [3] Ahmed N. Al-Niaimi, Ellen Hartenbach., "Intensive postoperative glucose control reduces the surgical site infection rates in gynecologic oncology patients", *Gynecol control*. 2015 January ; 136(1): 71–76.
- [4] Libman IM, Becker DJ (2003) Coexistence of type 1 and type 2 diabetes mellitus: "double" diabetes? *Pediatric Diabetes* 4: 110-113.
- [5] S. Vivekanandan , M.Devanand , "Remote monitoring for diabetes disorder: Pilot study using InDiaTel prototype," *European Research in Telemedicine/La Recherche Européenne en Télémedecine* ,Volume 4, (2015) pp. 63-69.
- [6] Cobelli C, Renard E, Kovatchev B (2011) Artificial pancreas: past, present, future. *Diabetes* 60: 2672-2682.
- [7] A. Alavudeen Basha, S. Vivekanandan , "Evolution of diabetic control identification in lieu of continuous glucose monitoring technology- A Review," *International Journal of Applied Engineering Research* ,Volume 12, Number 16 (2017) pp. 6102-6107.
- [8] Chee F, Fernando T (2007) *Closed-Loop Control of Blood Glucose*. 1st ed.Berlin Germany: Springer-Verlag.
- [9] Shah VN, Shoskes A, Tawfik B, Garg SK (2014) Closed-loop system in the management of diabetes: past, present, and future. *Diabetes Technol Ther* 16: 477-490.
- [10] R.N. Bergman, Y.Z. Ider, C. Bowden, and C. Cobelli: *Quantitative Estimation of Insulin Sensitivity*, American Physiological Society, Vol. 236, No. 6, pp. E667–E677, 1979.
- [11] A. Alavudeen Basha, S. Vivekanandan, "Optimal Control Identification of IMC and PID Controllers for Insulin Infusion," *CTCCEC IEEE conference* 2017.
- [12] Bergman RN, Urquhart J (1971) the pilot gland approach to the study of insulin secretory dynamics. *Recent Prog Horm Res* 27: 583-605 passim.
- [13] Bergman RN, Phillips LS, Cobelli C (1981) Physiologic evaluation of factors controlling glucose tolerance in man: measurement of insulin sensitivity and beta-cell glucose sensitivity from the response to intravenous glucose. *J Clin Invest* 68: 1456-1467.
- [14] Roy, A., "Dynamic Modeling of Free Fatty Acid, Glucose, and Insulin during Rest and Exercise in Insulin Dependent Diabetes Mellitus Patients," university of Pittsburgh, 2008.
- [15] Chen J., Cao K., Sun Y., Xiao Y., and Su X., "Continuous drug infusion for diabetes therapy: a closed-loop control system design," *Eurasip Journal on Wireless Communications and Networking*, vol. 2008.
- [16] Lehman E. D., Deutsch T., "The physiological model of glucose-insulin interaction in T1DM," *J. Biomed. Eng.*, 14:235–242, 1992.
- [17] Kamath S (2013) Model based simulation for type 1 diabetes patients. *Asian Am J Chem* 1: 11-19.
- [18] Kovács L, Szalay P, Benyó B, Chase G Applicability results of a nonlinear model-based robust blood glucose control algorithm. *J Diabetes Science Technol* 7: 708-716.
- [19] Magni L, Raimondo DM, Bossi L, Man CD, De Nicolao G, et al. (2007) Model predictive control of type 1 diabetes: an in silico trial. *J Diabetes Sci Technol* 1: 804-812.
- [20] Hovorka R, Canonico V, Chassin LJ, Haueter U, Massi-Benedetti M, et al. (2004) Nonlinear model predictive control of glucose concentration in subjects with type 1 diabetes. *Physiol Meas* 25: 905-920.
- [21] Dalla Man C, Rizza RA, Cobelli C (2006) Mixed meal simulation model of glucose-insulin system. *Conf Proc IEEE Eng Med Biol Soc* 1: 307-310.
- [22] Tanaka J.L.K., Wakasa Y., and Mizukami Y., "GA type IMC Control Pneumatic Servo System".

- Proceedings of SICE Annual Conference, Sapporo, Vol. 1 pp. 791-794, 2004.
- [23] Morari, M. and E. Zafiriou. (1989) Robust Process Control, Prentice-Hall, Englewood Cliffs, NJ.
- [24] B. Wayne Bequette "Process Control: Modeling, Design and Simulation (Prentice-Hall International Series in the Physical and Chemical Engineering Sciences)"
- [25] Rival and Personaz L., "Nonlinear Internal Model Control Using Neural Networks: Application to Processes with Delay and Design Issues," IEEE Transactions on Neural Networks, Vol. 11, No. 1, pp. 80-90, 2000.
- [26] Daniel E. Rivera and Melvin E., "Internal Model Control ," CONTROL SYSTEMS, ROBOTICS AND AUTOMATION - Vol. 2, pp. 01- 10, 1986.
- [27] Michael E. Fisher, "A Semi closed-Loop Algorithm for the Control Blood Glucose Levels in Diabetics", IEEE Transactions on Biomedical Engineering, vol.38, January,1991, pp:57-61.
- [28] Liu Jingkun. Advanced PID control and its Matlab simulation. Publishing house of electronics industry, 2003
- [29] Poterlowicz K., Hossain M.A., and Majumder M.A.A. "Optimal IMC System for Blood Pressure Control" in IEEE Proceeding of CS2007, ISSN: 1744-9170, pp. 113-117.
- [30] MATLAB SIMULINK, Simulink® Response Optimization™ 3User's Guide. The MathWorks, Inc. 2004-2008.
- [31] MATLAB SIMULINK, Simulink® Reference. The Math- Works, Inc. 2002-2008.
- [32] Roche (2015) Accu-ChekR Combo Training Handbook. Basel Switzerland:Roche.
- [33] Medtronic (2012) Mini Med R 530G System User Guide. Northridge, USA: Medtronic MiniMed.
- [34] Tandem (2012) t:slimR Insulin Pump User Guide. San Diego, USA: Tandem Diabetes Care.
- [35] Sherr J, Tamborlane W (2008) Past, present, and future if insulin pump therapy: A better shot at diabetes control. Mt Sinai J Med 75: 352-361.
- [36] Al-Tabakha MM, Arida AI (2008) Recent challenges in insulin delivery systems: a review. Indian J Pharm Sci 70: 278-286.

